



Technical data sheet TDS0100

HYDROCARBON INFRARED SENSOR Exd CERTIFIED VERSION TYPE MSH-HC



PATENT NUMBER: GB 2372099B; US 6,753,967 B2

FEATURES

- ★ ATEX, IECEx and UL Exd Certified for hazardous area use.
- ★ Measures methane at both % LEL levels and up to 100 % vol as well as general hydrocarbons in % LEL levels
- ★ Housing and internal optical paths constructed from stainless steel offering superior performance when compared to the earlier version HC/TC sensor
- ★ Direct replacement for HC/TC sensor
- ★ Optional, integral anti-condensation heater
- ★ Reduced baseline temperature dependency when compared to HC/TC sensor
- ★ Excellent baseline repeatability after temperature cycling
- ★ Minimum device to device temperature dependency variation
- ★ Standard sensor size
- ★ Temperature compensated detector elements
- ★ Fast Response
- ★ Internal temperature sensor to allow accurate temperature compensation
- ★ Low power
- ★ Gas diffusion sampling

Dynamant Limited

Hermitage Lane Industrial Estate · Kings Mill Way · Mansfield · Nottinghamshire · NG18 5ER · UK.

Tel: 44 (0)1623 663636 · Fax: 44 (0)1623 421063

email: sales@dynamant.com · www.dynamant.com

DESCRIPTION

Dynamant infrared sensors operate by using the NDIR principle to monitor the presence of target gas. The sensor contains a long life tungsten filament infrared light source, an optical cavity into which gas diffuses, a dual temperature compensated pyroelectric infrared detector and an integral thermistor to monitor the internal temperature. The infrared source should be driven externally with a constant voltage supply switched at a fixed frequency with a 50% duty cycle. The dual pyroelectric detector produces two output signals in response to pulsed incident radiation from the source:

- An active signal which decreases in the presence of target gas
- A reference signal which is used to monitor the intensity of the source

Both signals are composed of a DC offset voltage (typically 0.7V – 1.0V) with a small superimposed response signal alternating in sympathy with the source drive voltage. The alternating signal must be extracted and amplified in order to obtain a measure of the peak to peak value for both the active and reference. The ratio of active to reference peak to peak signals is essentially independent of variations in source intensity over time and this ratio reduces in the presence of target gas. It is the reduction in this ratio that is used to determine the target gas concentration. The reduction in ratio is non-linear and the gas concentration can be extracted using the expression:

$$[\text{concentration}] = (-\ln (1 - (1 - \text{Ratio}/\text{zero})/\text{span})) / a)^{1/b}$$

Where **zero** is the ratio in the absence of target gas, **span** is determined during calibration & the constants **a** and **b** are:


a = 0.022989, **b** = 0.78836 and typical **span** = 0.2 for a range of 0-100%l/l methane.

a = 0.020748, **b** = 0.500 and typical **span** = 2.5 for a range of 0-100% volume methane.


a = 0.0118, **b** = 0.911 and typical **span** = 0.7 for a range of 0-100%l/l non-methane aliphatic hydrocarbons (eg propane)


The internal temperature signal is used to measure the temperature inside the sensor. This temperature measurement is used to correct for the ideal gas law and also to correct for any optical filter effects on zero and span as a function of temperature. The internal temperature is typically 8°C higher than ambient at 20°C due to the heat generated from the infrared source. This internal heating beneficially reduces the probability of water condensing within the optical cavity.

Further details on the sensor, interfacing circuitry, signal extraction and relative responses to other hydrocarbons can be found in the Dynamant application notes on the Dynamant web site or by contacting Dynamant directly.



Notes: The above graph is based on 5% volume methane = 100% LEL
 The response curves show typical responses, there will be a variation from sensor to sensor.

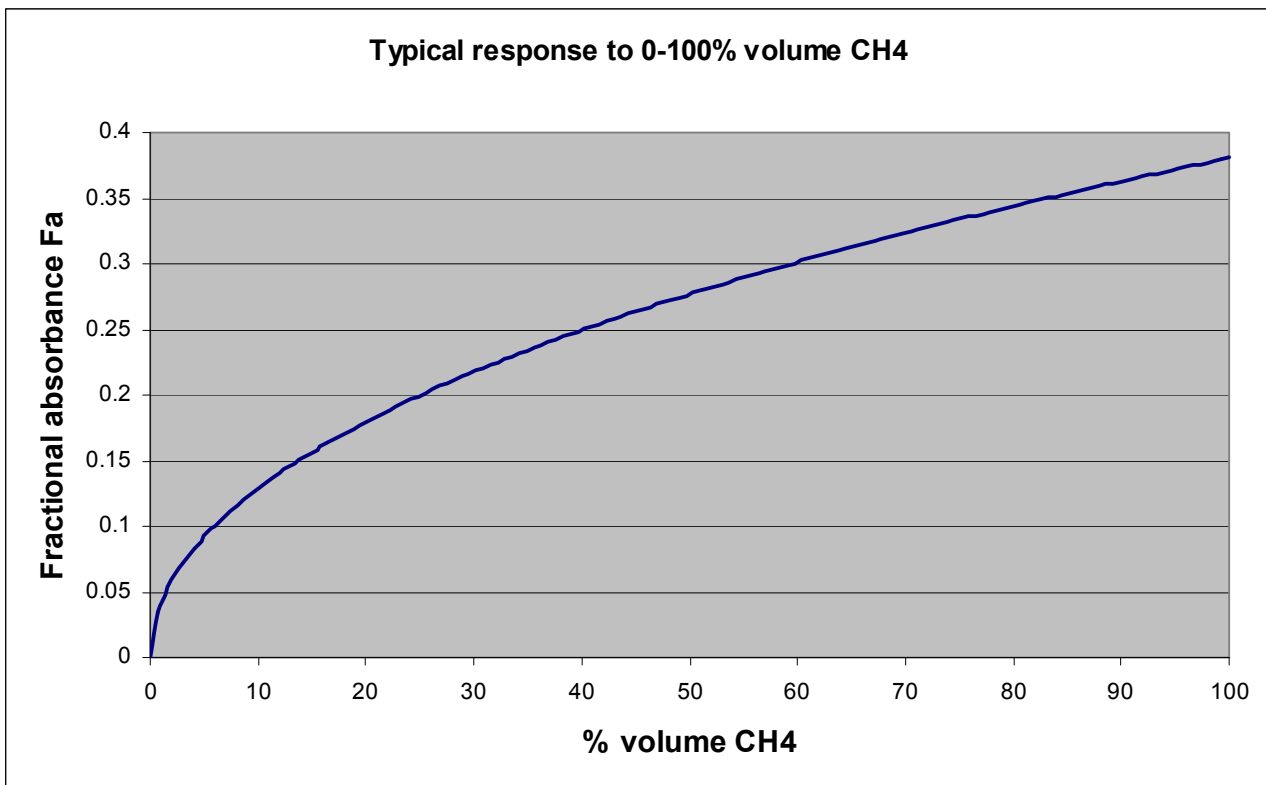

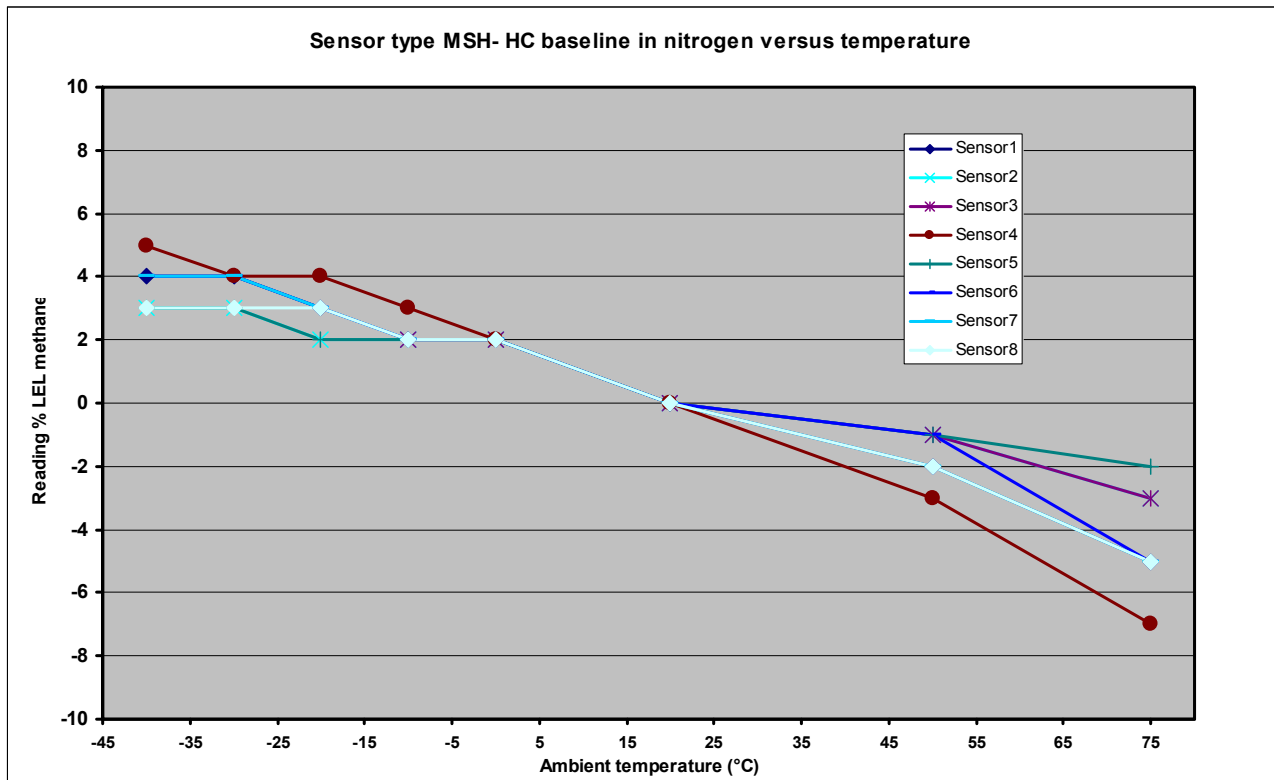

The above graph shows the baseline temperature dependency, and device to device variation for a sample of eight sensors tested from -40 °C to +75 °C.

Note that the warranty and certification limit the temperature range to -20 °C to +50 °C.

OPTIONAL ANTI-CONDENSATION HEATER

Under certain operating conditions it is possible for condensation to take place on the optical paths of the sensor. This will cause temporary inaccuracies in the sensor outputs. Condensation can occur when the gas sample is high in humidity, and at a higher temperature than the internal optical surfaces of the sensor. In order to prevent condensation the optical surfaces need to be a few degrees Celsius above the temperature of the gas sample. The addition of a heating resistor embedded within the epoxy encapsulation of the sensor raises the sensor's working temperature, in free air, by approximately 8°C above ambient temperature. Without the heating resistor the sensor's working temperature is 4°C above ambient temperature.

The heating resistor is fitted across the lamp supply and has a value of 120 ohms. With a 5V lamp supply voltage the resistor will dissipate 0.21W and draw an additional 42 mA from the supply.

For applications where the additional lamp current cannot be delivered by the drive circuit, an alternative arrangement is available with the heating resistor fitted across the supply to the pyroelectric device. Refer to the "Example of Ordering Codes" for further information on how to specify the heating options.

TEMPERATURE COMPENSATION

Pyroelectric devices exhibit a certain degree of temperature dependency; this is largely due to the band pass filter characteristics. For this reason, it is necessary to apply temperature compensation to the values used to calculate the gas readings.

Temperature compensation can be applied to the **Zero factor** and to the **Span factor**, depending upon the sensor type. Typically hydrocarbon sensors require only **Zero factor** temperature compensation whereas carbon dioxide sensors require **Span factor** temperature compensation.

The closely matched temperature dependency of the HC sensors make it possible to apply a single value of temperature compensation to the “Zero factor” thereby improving accuracy, and eliminating the need to apply individually calculated values for each sensor.

The following temperature compensation technique is provided as a guide, end-users may employ other procedures that are more appropriate to their specific applications.

Zero factor temperature compensation.

The way in which the zero factor temperature compensation is used to correct the reading is as follows:

Zero factor = Zero factor X (1.0 + (Temperature offset X Zero Temperature Compensation value))

Where Temperature offset = Current temperature – Zero temperature

Span factor temperature compensation.

The way in which the span factor temperature compensation is used to correct the reading is as follows:

Span factor = Span factor X (1.0 + (Temperature offset X Span Temperature Compensation value))

Where Temperature offset = Current temperature – Span temperature

The reading is now calculated using the formula provided in Application Note AN0003.

An approximation to the *Ideal Gas law* is then applied to the reading as follows:

Reading = Reading without correction X Temperature offset

Where Temperature offset = (Current temperature + 273.15) / (Span temperature + 273.15)

Summarising:


- 1) The **Zero factor** is corrected for temperature.
- 2) The **Span factor** is corrected for temperature.
- 3) The reading is calculated.
- 4) The reading is adjusted using the ideal gas law.

The table below shows typical temperature compensation values for the HC sensors when used with the Dynamet OEM gas transmitter type OEM-1.


Gas type	Zero Temperature Compensation	Span Temperature Compensation
5% CH ₄	-0.0002	0
100% CH ₄	-0.0002	0



It should be noted that the Temperature Compensation values above represent the combined temperature behaviour of both the sensor and the associated electronic circuitry. It is recommended that manufacturers perform their own temperature tests to validate the performance of their equipment over the required operating temperature range.

**Sensor type MSH-HC baseline variation over temperature,
NO temperature compensation applied**



**Sensor type MSH-HC baseline variation over temperature,
Zero factor temperature compensation value of -0.00020 applied**





These graphs show the effect of applying a single value of “zero factor” temperature compensation to eight sensors, tested over the range -20°C to +50°C

SPECIFICATION

Maximum lamp Power Requirements:	5V d.c. 60mA max. (50% duty cycle source drive)
Minimum operating voltage:	3.0V d.c. (50% duty cycle source drive)
Source drive frequency :	2.0Hz minimum, 3.0 Hz typical, 4.0 Hz maximum
Active mV pk-pk output in N₂:	12.0mV typical @ 3Hz, 50% duty cycle
Reference mV pk-pk output in N₂:	4.0mV typical @ 3Hz, 50% duty cycle
Sensitivity (reduction in active signal) at 20°C, 4Hz, 50% duty cycle:	11% typical @ 5% vol. CH ₄ 36% typical at 100% volume CH ₄ 18% typical @ 1.7% vol. propane
Methane measuring range:	0 – 5% volume up to 0 – 100% volume
Hydrocarbon measuring range	0 – 100% LEL
Resolution:	1% of measuring range (dependent upon signal processing)
Warm up time:	To final zero ± 2% LEL : <20s @20°C (68°F) ambient To specification: < 30 minutes @20°C (68°F) ambient
Response Time T₉₀:	<30s @20°C (68°F) ambient
Zero Repeatability:	± 1% LEL CH ₄ @20°C (68°F) ambient
Zero Repeatability after temperature cycling:	± 2% LEL CH ₄ after cycling from -20°C to +50°C (Based on data from eight sensors cycled eight times)
Span Repeatability:	± 2% LEL CH ₄ @20°C (68°F) ambient
Long term zero drift:	± 1% LEL CH ₄ per month @20°C (68°F) ambient
Operating temperature range:	-20°C to +50°C (-4°F to 122°F)
Storage temperature range	-20°C to +50°C (-4°F to 122°F)
Humidity range:	0 to 95% RH non-condensing.
MTBF	> 5 years
Temperature signal	Integral thermistor for temperature monitoring
Weight :	17 grams

MECHANICAL DETAIL

NOTES

- TOLERANCE +/- 0.15 UNLESS OTHERWISE STATED
- RECOMMENDED PCB SOCKET: WEARNES CAMBION LTD CODE: 450-3326-01-06-00
- WEIGHT: 15g
- USE ANTI-STATIC PRECAUTIONS WHEN HANDLING**
- DO NOT CUT PINS**
- DO NOT SOLDER DIRECTLY TO PINS**
- THE LABELLING ADDS UP TO 0.2 TO THE OUTER DIAMETER AND UP TO 0.2 TO THE OVERALL HEIGHT

PIN OUT

- LAMP RETURN
- LAMP +5V
- +5V PYRO SUPPLY
- DETECTOR OUTPUT
- REFERENCE OUTPUT
- THERMISTOR OUTPUT
- 0V PYRO SUPPLY AND CASE CONNECTION

Available sensor options:

L XXX = Heater on lamp supply, plus value in ohms

P XXX = Heater on pyroelectric supply, plus value in ohms

P = Removable 45 micron plastic insert dust filter

F = Replaceable, self adhesive porous PTFE filter

I = Case isolated from 0V pin

EXAMPLE OF ORDER CODES

MSH- HC / L XXX / P / F / I

OPTIONS

- ISOLATION BLANK = STANDARD
I = ISOLATED CASE
- FILTER BLANK = OMITTED
F = FITTED
- PLASTIC INSERT BLANK = OMITTED
P = FITTED

L = Heater on lamp supply, value XXX ohms
P = Heater on pyroelectric supply, value XXX ohms

GAS TYPE : HC = Hydrocarbon

CERTIFICATION DETAILS

European ATEX Certification

Approval body	SIRA
Certificate Number	SIRA 04ATEX1357U
Test Standards	EN60079-0:2009, EN60079-1:2007, EN60079-11:2007, EN60079-26:2007
Certification Codes	I M2 Ex d I Mb II 2 G Ex d IIC Gb
Input parameters	0.8W max, 30V max. (See footnote)
Operating temperature	-20°C to +60°C (See footnote)

International IECEx Certification

Approval body	SIRA
Certificate Number	IECEx SIR 05.0053U
Test Standards	IEC 60079-0:2007-10, Edition 5 IEC60079-1:2007-4, Edition 6 EN60079-26:2006 Edition 2
Certification Codes	Ex d I and/or Ex d IIC
Input parameters	0.8W max, 30V max.
Operating temperature	-20°C to +60°C (See footnote)

North American Certification

Approval body	Underwriters Laboratory Inc.
File Reference	E336365
Test Standards	UL 60079 – 0, 4 th Edition UL 60079 - 1, 6 th Edition CAN/CSA-C22.2 No. 60079-0-1-7 CAN/CSA-C22.2 No. 60079-1 part 1, 1 st Edition
Hazardous Locations	Class 1, Zone 1, AEx d IIC and Ex d IIC Hazardous Locations
Input/Entity parameters	0.8W max, 30V max.

Input parameters are defined for certification purposes only, refer to the "Specification" table for the sensor operating voltage and temperature range.

Warranty information

All Dynament Standard sensors carry a two year warranty against defects in materials and workmanship. The warranty is invalidated if the sensors are used under conditions other than those specified in this data sheet.

Particular attention should be paid to the following criteria:

- **Observe the correct supply polarity**
- **Do not exceed the maximum rated lamp supply voltage of 5V**
- **Do not solder directly to the sensor pins**
- **Do not expose the sensor to corrosive gases such as hydrogen sulphide**
- **Do not allow dust or liquids to enter the sensor**
- **Do not exceed the operating temperature range**